Lafil 100 / Lafil 100eco

Portable Suction System

Important Notice

- Read and comply with this manual before installing or operating the equipment.
- Please ensure that the power supply voltage matches the voltage rating for the instrument.
- Please operate the instrument in well ventilated area and keep away from inflammables.
- This instrument is not corrosion-proof pump. It is not suitable for pumping acid, base or organic vapors or gases directly.
- Do not modify the equipment without authorization.
- Clean and maintain the instrument and accessories according to the maintenance method after every use.


Unpacking

Carefully check if the shipping carton is damaged before unpacking. Please check the items according to standard package list. If you have any questions, please preserve serial number, shipping carton and contact your dealer for quick solution.

Position	Designation	
1	Lafil 100 / Lafil 100eco suction unit	
2	Handle	
3	1 channel tip adaptor with ejector	
4	8 channel tip adaptor with ejector	
5	1000 ml Vacuum bottle with	
	GL45 Suction cap	
6	Disc filter	
7	30 cm Silicone tube	
8	200 cm Silicone tube	
9	Power adapter	
10	Accessory kit	
11	Instruction manual	




Assembly & Disassembly diagram

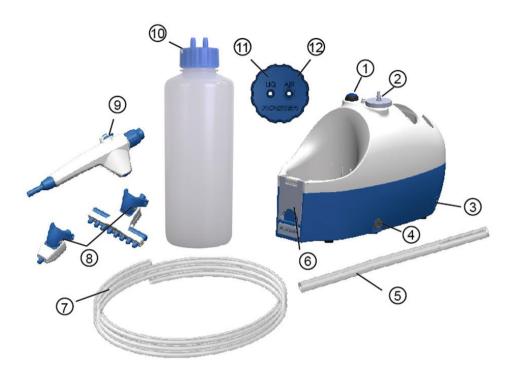

Position	Designation
1	Power switch
2	Disc filter
3	Residual liquid collection tray
4	Power plug
5	30 cm silicone tube (short)
6	Centrifuge tube rack
7	200 cm silicone tube (long)
8	Ejector bottom
9	Lock switch
10	1000 ml Vacuum bottle with GL45 Suction cap
11	"LIQ" hose barb of the suction cap
12	"AIR" hose barb of the suction cap

Installation and Operation

Lafil 100 / Lafil 100eco Assemble the disc filter and the residual liquid collection tray in Lafil 100 or Lafil 100eco suction unit. Assemble the vacuum bottle set as the figure, then put it on the suction unit. Assemble the short tube with the disc filter to the "AIR" hose barb of the suction cap. Assemble the long tube with the handle to the "LIQ" hose barb of the suction cap Connect the power supply and switch on the power. Choose the suitable adaptor to connect with the handle. You can press the lock switch to do operation continuously. You can press the ejector bottom to eject tips.

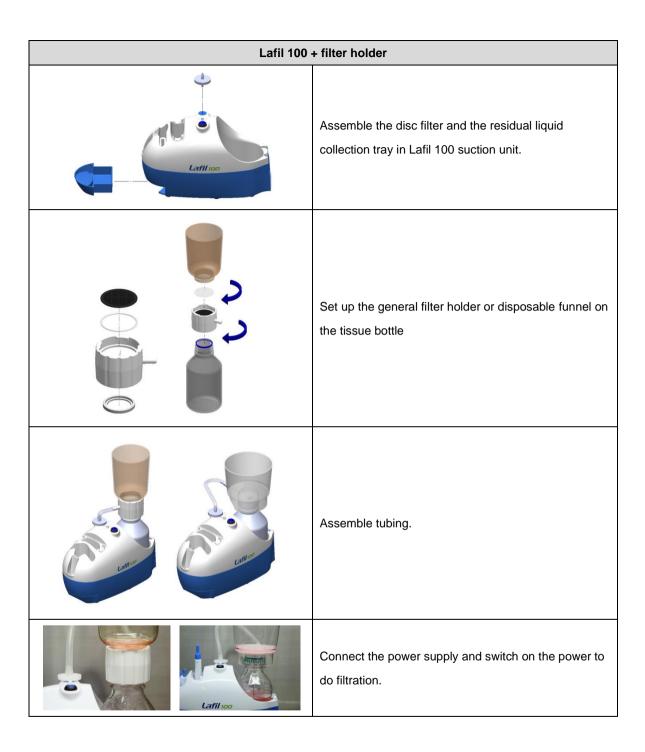

Maintenance

- 1. Please suck in pure water to clean the tubing after every use.
- 2. Suction accessories and silicone tube are autoclavable. Please clean and autoclave if needed.
- Lafil 100 and Lafil 100^{eco} suction unit is not autoclavable. Please clean the case by pure water or 75% alcohol.
- 4. It is strongly recommended to replace the main parts (internal rubber adaptor, O-ring and SS spring) of the handle every year at least to keep good aspiration.
- 5. Disc filter and silicone tubes are consumables, please replace at least every half year to ensure good aspiration.

Troubleshooting

Symptoms	Possible causes	Remedy
	No electrical supply	Check the power supply conform to
		power specified on main unit or the
Instrument fails to start		switch is broken
	2. Power switch off	Switch on power
	3. High vacuum still	Release the vacuum
	1. Air outlet clogged	Clean or replace the air outlet
Manusca faile to adjust	2. Weak power supply	Check the power supply
Vacuum fails to adjust	3. Leak in the system	Check tubing, seals and coupling,
		replace if necessary
	1. Leak in the system	Check tubing, seals and coupling,
Law Chartier and divine		replace if necessary
Low filtration speed/ poor	2. Liquid overflow	Check if the suction bottle is overflowing
vacuum	3. Weak power supply	Check the power supply
	4. Filter clogged	Replace filter

Ordering Information

197100-01	Lafil 100, Portable Suction System with AC100-240V adaptor, US plug
197100-02	Lafil 100, Portable Suction System with AC100-240V adaptor, EU plug
197100-03	Lafil 100, Portable Suction System built-in battery with AC100-240V adaptor, US plug
197110-01	Lafil 100eco, Portable Suction System with AC100-240V adaptor, US plug
197110-02	Lafil 100eco, Portable Suction System with AC100-240V adaptor, EU plug
199100-30	Handle
199100-75	1-channel tip adaptor with ejector (for 200 µl tip)
199100-50	8-channel tip adaptor with ejector (for 200 μl tip)
197100-47	1-channel SS adaptor (40 mm)
197000-48	1-channel S adaptor (80 mm)
197100-49	8-channel SS adaptor (40 mm)
197000-02	LF 3a, 300ml PES filter holder
197000-04	LF 5a, 500ml PES filter holder
197100-48	Anti-UV Cloth Cover
197100-10	1000 ml PP vacuum bottle
197000-60-500	500 ml glass bottle with GL45 suction cap