

INSTRUCTION MANUAL

Oil Free Vacuum Pump and Compressor


Model No.

Rocker 300 / 300DC / 400 / 410

Rocker 900 / 901 / 910 / 911

Rocker 430

Tech support

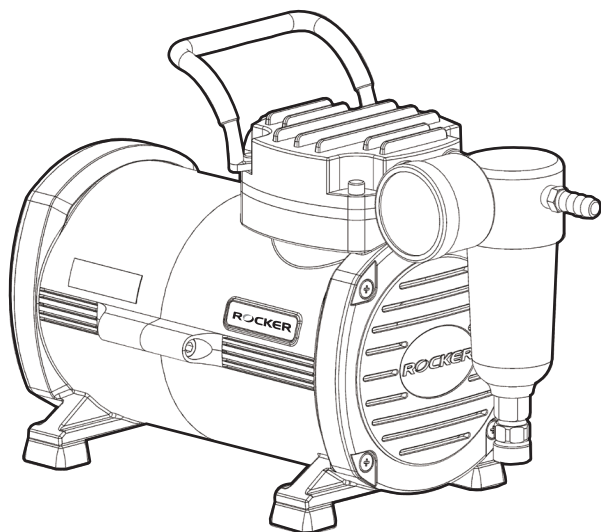

ROCKER

Please read this instruction manual before using this product.

Important Notice

This instrument is designed for laboratory usage only. Please read this manual carefully before installing and operating. The instrument shall not be modified in any way. Any modification will void the warranty and may result in potential hazard. We are not responsible for any injury or damage caused by any non-intended purposes and modifying the instrument without authorization.

1. Check the voltage specified on the name plate and ensure it matches the line voltage in your location.
2. Install the instrument in a clean, dust-less and ventilated area under 40°C.
3. Never use the instrument with any corrosive, chemical, flammable gas or toxic material.
4. Please connect the instrument with high-pressure hose or tubes.
5. The Prote™ filter cartridge can prevent a large amount of liquid from overflowing into the pump. Please ensure the liquid in the moisture trap not exceed safety level.
6. To ensure proper function of the Prote™ protection device, the pump must be installing on a flat level surface and should not be moved when operation. If the buoy closes during operation, it must be manually reset by uninstalling and reinstalling the filter cartridge.
7. The filter cartridge is used to absorb moisture and block dust. Please replace the cartridge to maintain pumping efficiency when it becomes dirty or color-changing.
8. The instrument is not designed to start against applied vacuum / pressure. To prevent damage, verify that the inlet and outlet are at atmospheric pressure before each start. If necessary, the inlet (and outlet of Rocker 430) can be vented to atmosphere by partially unscrewing the regulator knob.
9. This instrument has a thermal protection device that automatically shuts-off when it becomes overheated.
10. The temperature of the instrument surface is very high after use or during work, please don't touch it to avoid being burnt.
11. The instrument must not be used to create vacuum and pressure simultaneously.
12. Do not use any lubricant, which may damage the instrument.
13. If the supply cord is damaged, please contact the manufacturer or your service agent for replacement to avoid hazard.

14. Please discard packing material according to local related regulations.

15. Operating condition

(a) Ambient temperature: 5~ 40°C

(b) Relative humidity: 80% RH Max.

(c) Power supply: 100-120V~, 50/60Hz or 200-240V~, 50/60Hz

(d) Altitude: up to 2000 m

(e) Pollution degree: II

(f) Indoor use



Caution: Hot surface

****Warning: While Rocker 430 is operated as a compressor, please ensure a 20-min break while every 30-min working to prevent the instrument shutdown from overheating.***


Unpacking

Please check if the package is complete without any damage before unpacking. When unpacking, please make sure you have all accessories that indicated on the list. If there is any problem, please keep the serial number along with packing case and contact your local distributor immediately for assistance.


Main Part Diagram

• Vacuum Pump

Rocker 300

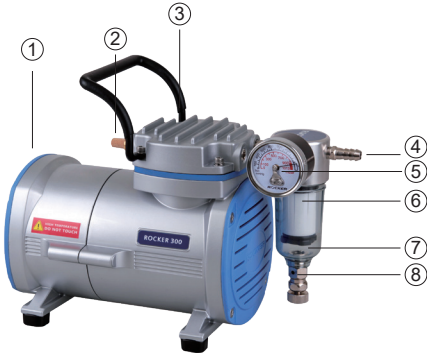


Rocker 300DC

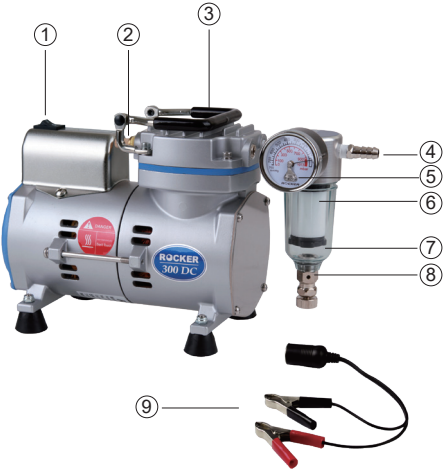


| Position | Designation | Position | Designation |
|----------|----------------------|----------|-------------------------|
| 1 | Power Switch | 6 | Prote™ Filter Cartridge |
| 2 | Air Outlet (Muffler) | 7 | Moisture Trap |
| 3 | Handle | 8 | Vacuum Regulator |
| 4 | Air Inlet | 9 | Power Cord |
| 5 | Vacuum Gauge | | |


* The reference point of vacuum gauges is atmospheric pressure.

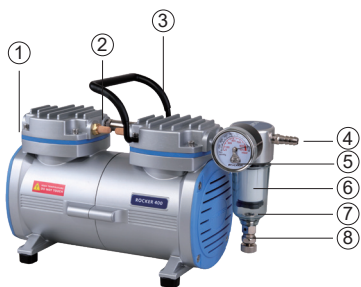


Rocker 400

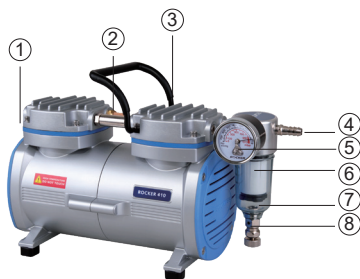

Rocker 410

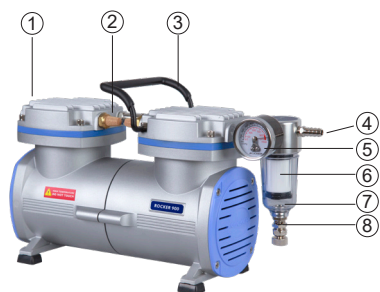

Rocker 900

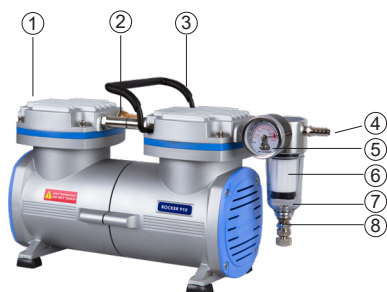

Rocker 910

| Position | Designation | Position | Designation |
|----------|----------------------|----------|--------------------------|
| 1 | Power Switch | 5 | Vacuum Gauge |
| 2 | Air Outlet (Muffler) | 6 | Prote™ Filter Cartridge* |
| 3 | Handle | 7 | Moisture Trap |
| 4 | Air Inlet | 8 | Vacuum Regulator |

* Rocker 900 / 910 is equipped with only filter cartridge, no Prote™ protection device.




Rocker 901



Rocker 911

• Vacuum Pump and Compressor

Rocker 430

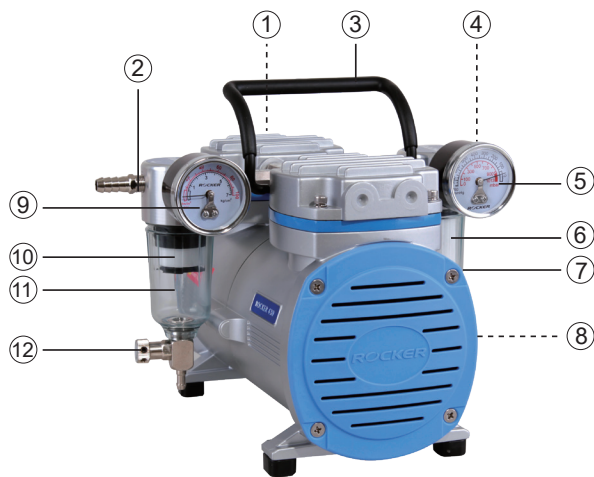

| Position | Designation | Position | Designation |
|----------|----------------------------|----------|----------------------------------|
| 1 | Power Switch | 7 | Moisture Trap |
| 2 | Air Outlet (Pressure Side) | 8 | Vacuum Regulator |
| 3 | Handle | 9 | Pressure Gauge |
| 4 | Air Inlet (Vacuum Side) | 10 | Filter Cartridge |
| 5 | Vacuum Gauge | 11 | Moisture Trap |
| 6 | Prote™ Filter Cartridge | 12 | Pressure Regulator (Drain Valve) |

* The reference point of both vacuum and pressure gauges is atmospheric pressure.

Operation

• Operation

- A. Press power switch (1) to activate the instrument after making sure all tubing are well connected.
 - A cold trap or trap bottle is recommended to connect before air inlet (4) of vacuum pump, while amount of moisture and steam exists.
- B. To setup vacuum by adjusting the vacuum regulator (8).

Pressure can also be set up on Rocker 430 by adjusting the pressure regulator (12).

 - Pilot 100, vacuum controller (Cat. No. 183100-01(02)) is available for precise vacuum control.
- C. Check liquid level of moisture trap (7) daily and drain the liquid when it is up to the neck of bottle.

* Warning:

(1) When pump is used for aqueous solution filtration, please ensure the liquid level of flask not exceed safety level. Failure to comply could result in serious damage to the pump and void the warranty. If it occurs, please contact the distributor immediately for service.

(2) While Rocker 430 is operated as a compressor, please ensure a 20-min break while every 30-min working period to prevent the instrument shutdown from overheating.



Filtration System Assembly Diagram

Maintenance

1. Please remove the liquid in the moisture trap after every use and keep pumping the air for at least 2 minutes to withdraw the residual steam.
2. If the liquid in moisture trap is more than 70%, please stop the experiment immediately to empty the liquid.
3. The instrument is not autoclavable. Please clean the surface by pure water or 75% ethanol.
4. Please replace the cartridge to maintain pumping efficiency when it becomes dirty or color-changing.
5. Valve plate(s), O-ring(s) and silicone tube(s) are consumables, it is recommended to replace it on a yearly basis or as needed to ensure good operation.

• How to reset the Prote™ protection device

1. Remove the moisture trap (7) and filter cartridge (6) by rotating clockwise.
2. Disassemble the filter cartridge (6) to ensure the buoy is not closed.
3. Reinstall all components, filter cartridge and moisture trap back.

• How to replace cartridge

1. Please replace the cartridge when it becomes dirty or color-changing.
2. Please remove the moisture trap (7 / 11) by rotating it clockwise.
3. Replace the cartridge by the same way.

Troubleshooting

| Problem | Reason and Solution |
|------------------------|--|
| Failed to start | <ul style="list-style-type: none">● Loose plug → Reconnect plug to power supply.● Wrong voltage → Reconnect to power specified on name plate.● Vacuum or pressure exists → Release vacuum / pressure and restart.● Switch is broken → Contact distributor for assistance. |
| Poor vacuum / pressure | <ul style="list-style-type: none">● Improperly vacuum / pressure setting → Adjust the regulator.● Faulty gauge → Replace a new gauge.● Air leakage → Replace or tighten the tubing and accessories that possible leaks. |

Ordering Information

| | |
|---------------|--|
| 167300-11(22) | Rocker 300 Vacuum pump, AC110V,60Hz (AC 220V,50Hz) |
| 167300-00 | Rocker 300DC Vacuum pump, DC12V |
| 167400-11(22) | Rocker 400 Vacuum pump, AC110V,60Hz (AC 220V,50Hz) |
| 167410-11(22) | Rocker 410 Vacuum pump, AC110V,60Hz (AC 220V,50Hz) |
| 167430-11(22) | Rocker 430 Vacuum Pump / Compressor, AC110V,60Hz (AC 220V,50Hz) |
| 167900-11(22) | Rocker 900 Vacuum pump, AC110V,60Hz (AC 220V,50Hz) |
| 167901-11(22) | Rocker 901 Vacuum pump, AC110V,60Hz (AC 220V,50Hz) |
| 167910-11(22) | Rocker 910 Vacuum pump, AC110V,60Hz (AC 220V,50Hz) |
| 167911-11(22) | Rocker 911 Vacuum pump, AC110V,60Hz (AC 220V,50Hz) |
| 183100-01(02) | Pilot 100, Vacuum Controller, AC100-240V adaptor, US plug (EU plug) |
| 167301-06 | Moisture trap / Vacuum regulator for Rocker 300 / 400 / 410 / 430 |
| 167301-07 | Prote™ filter cartridge for Rocker 300 / 400 / 410 / 430 |
| 167300-42 | Muffler (Air outlet) for Rocker 300 / 400 / 410 |
| 167801-06 | Moisture trap / Vacuum regulator for Rocker 900 / 910 |
| 167801-07 | Filter cartridge for Rocker 900 / 910 (without Prote™ overflow protection) |
| 167600-42 | Muffler (Air outlet) for Rocker 900 / 901 / 910 / 911 |
| 167320-06 | Moisture trap / Pressure regulator for Rocker 320 / 420 / 430 (Pressure side) |
| 167300-07 | Filter cartridge for Rocker 320 / 420 / 430 (Pressure side) |
| 167300-21 | Hose barb, 1/8 PT, 5/16 in. for Rocker 300 / 300DC / 400 / 410 / 430 / 900 / 910 |
| 167300-20 | Hose barb, 1/4 PT, 3/8 in. for Rocker 901 / 911 |
| 167200-38 | Silicone Tube, Ø 6 x 12 mm, 1 m |
| 180300-68 | Silicone Tube, Ø 8 x 14 mm, 2 m |

• Rocker Pump Repair Kit

| | | | |
|-------------|-----------------------|-----------|-----------------------|
| 167300-62-1 | Rocker 300 repair kit | 167900-62 | Rocker 900 repair kit |
| 167400-62-1 | Rocker 400 repair kit | 167901-62 | Rocker 901 repair kit |
| 167410-62-1 | Rocker 410 repair kit | 167910-62 | Rocker 910 repair kit |
| 167430-62 | Rocker 430 repair kit | 167911-62 | Rocker 911 repair kit |

Rocker Scientific Co., Ltd.

Tel: +886-2-26033311 Fax: +886-2-26036622

E-mail: export@rocker.com.tw <https://www.rocker.com.tw>